

1. Operating instructions notes

These operating instructions for the Endecotts test sieving machines give all necessary information on the sections mentioned in the contents.

They give instructions to the target group(s) defined in the respective sections for safe, correct handling of the Endecotts machines. It is important that each target group(s) is (are) familiar with the relevant section, in order to ensure safe, reliable handling of the machine according to its intended use.

This technical documentation is for use as a reference work and as a learning aid.

The information of each individual product (sieving machines) is complete within their section.

Repair instructions are not included in this manual. If repairs are necessary please contact your supplier or Endecotts Ltd directly.
Endecotts Ltd www.Endecotts.com

Warnings

The following signs are used to warn of hazards:



Personal injuries



Material damage

Safety

Target group:

All persons concerned with the machine in any way.

The entire Endecotts machine range is a modern, highly efficient product of Endecotts Ltd, corresponding to state of the art works. If the machine is used according to the intended purpose with knowledge of this technical documentation it is completely safe and reliable to operate.

Safety instructions

As the operator it is your duty to ensure that all persons charged with working on the Endecotts machine:

- Have read and understood all the instructions on safety,
- Before beginning work know all the instructions and regulations for the target group relevant to their work,
- Have access to the technical documentation for this machine at all times, without problems.
- New personnel should be familiarised with safe, proper handling of the machine before beginning work on the Endecotts machine, either by verbal instruction from a competent person or through this technical documentation.
- Improper operation can cause injury to persons or damage to the equipment. You are responsible for your own safety and that of your employees.
- Ensure that unauthorised persons have no access to the Endecotts machine.

For your own protection have your employees confirm that they have been instructed in operation of the Endecotts machine. The draft of a suitable form is given at the end of the section on safety.



We exclude claims for damages in any form for damage to persons or property caused through non-observance of the following safety instructions.

Summary of safety instructions

Safety instructions



We exclude claims for damages in any form for damage to persons or property caused through non-observance of the following safety instructions.

Technical data



Do not make any changes to the machine and use only spare parts and accessories which have been approved by Endecotts.
The declaration of conformity to the European directives by Endecotts will otherwise lose its validity. Furthermore this will result in the loss of any kind of guarantee claims.

Packing



Please keep the packing material during the guarantee period in case of a complaint your guarantee claim will be at risk if the machine is returned in inadequate packing.

Transport



The **Endecotts machine** must not be knocked, shaken or thrown during transport; otherwise the electronic and mechanical components may be damaged.

Temperature fluctuations



If subjected to high temperature fluctuations (e.g. during transport by plane) the **Endecotts machine** must be protected against condensed water. If not damage to the electronic components may be caused.

Supply schedule



If the delivery is incomplete and/or transport damage has occurred, you must immediately notify the transport agent and Endecotts Ltd (within 24 hrs.). It is possible that later complaints may not be considered.

Ambient temperature



If the ambient temperature is exceeded or drops below the normal value the electrical and mechanical components may become damaged and the performance data can change to an unknown degree.

Atmospheric humidity



At high atmospheric humidity the electrical and mechanical components may become damaged and the performance data can change to an unknown degree.

Installation / transport protection - IMPORTANT



If the machine is operated with the transit bolts, or is transported without transit bolts, mechanical components may become damaged.

Electrical connection / connecting the mains power supply



If the values given on the rating label are not observed electrical and mechanical components may become damaged.

Wet sieving



Never operate your **Endecotts machine** directly in water.
Danger through current surge.



During wet sieving always operate your **Endecotts machine** connected to a mains socket which is protected by an FI protective (safety) switch.



The water quantity added should always be dosed in such a way that the sieve surface is only just wetted.

Sieving aids



Make sure that the wire mesh of the sieves is not excessively stretched through overloading with sieving aids, since this will impair the precision of your test sieves.



Damage may occur if the shaker is allowed to operate with a loose clamping plate.

Cleaning



Do not clean the **Endecotts machine** under running water.
Danger to life through current surge.
Use only a cloth moistened with water; solvents are not allowed.

Wearing parts



These operating instructions do not include repair instructions.
For your own safety, repairs should be carried out only by Endecotts Ltd or an authorised agency or Endecotts service technicians.

Confirmation

I have read and taken note of the sections – preliminary
comments and safety

Signature of operator

Signature of service technician

5. Operating instructions: Octagon 200CL



Technical specifications

SIEVE SHAKER MODEL:

Octagon 200CL

General Information

The new Octagon 200CL for precise, reproducible and error-free sieving processes competes with the most advanced sieve shakers in the world. Several unique features have been developed specifically for this machine, including the 'Closed Loop' amplitude control for ultimate reproducibility. The Octagon 200CL is designed to work with Endecotts SieveWare, the new software for easy evaluation and documentation of the sieving process.

Advantages

- 'Closed Loop' total amplitude control ensures reproducible sieving
- Digital controls for easy and reliable operation
- Easy-to-use sieve clamping system
- Accepts up to 8 full height 200 mm or 8" diameter sieves
- Suitable for dry and wet sieving
- 3D sieving motion allows for high separation efficiency and non-blinding sieving action
- Full compatibility with new SieveWare evaluation and control software via RS232 Port (printed or digital protocols)
- Voltage-independent
- No mechanical moving parts
- Compact and portable



Do not make any changes to the machine and use only spare parts and accessories approved by Endecotts Ltd.

The declaration of conformity to the European directives by Endecotts will otherwise lose its validity.

Furthermore this will result in the loss of any kind of guarantee claims.



Specifications

Range	20 µm to 125 mm
Drive / sieving motion	electromagnetic 3D
Max. Batch / feed capacity	3 kg
Max. Number of fractions	8 full height / 16 half height (200 mm or 8")
Amplitude	0 - 3 mm digital setting in 0.1 mm steps " Closed Loop" amplitude control
Speed	3,000 min ⁻¹ at 50 Hz
Time display	digital, 0:10-99:50 min
Interval operation	yes (two modes)
Suitable for dry sieving	yes
Suitable for wet sieving	yes
Serial interface	yes (RS232)
Sieve diameter	100 / 200 mm or 3" / 8"
Max. Height of sieve stack	up to 450 mm
Clamping device	quick-release clamping system (included)
Model	bench top
Protection code	IP 54
Electrical supply	100-240V 50/60Hz
Power connection	1 - Phase
W x H x D	418 x 232 x 435 mm
Net weight	35 kg
Standards	CE

Noise characteristic values:

Example 1:

Emission value related to workplace L_{pAeq} = 63 dB (A)

(Operating conditions: Material to be sieved = quartz sand, grain size < 1mm, 5 sieves Amplitude = 1.5 mm)

Example 2:


Emission value related to workplace L_{pAeq} = 67 dB (A)


(Operating conditions: Material to be sieved = quartz sand, grain size < 1mm, 5 sieves Amplitude = 3 mm)

Controls and functions

The sieve shaker should be placed on a level surface to ensure symmetrical distribution of the sample over the sieve mesh. The surface should be rigid and robust where vibration will not cause problems.

Operators should be familiar with and fully understand the controls and indicators before operating this machine. This should be done in conjunction with the diagram below and control panel description.

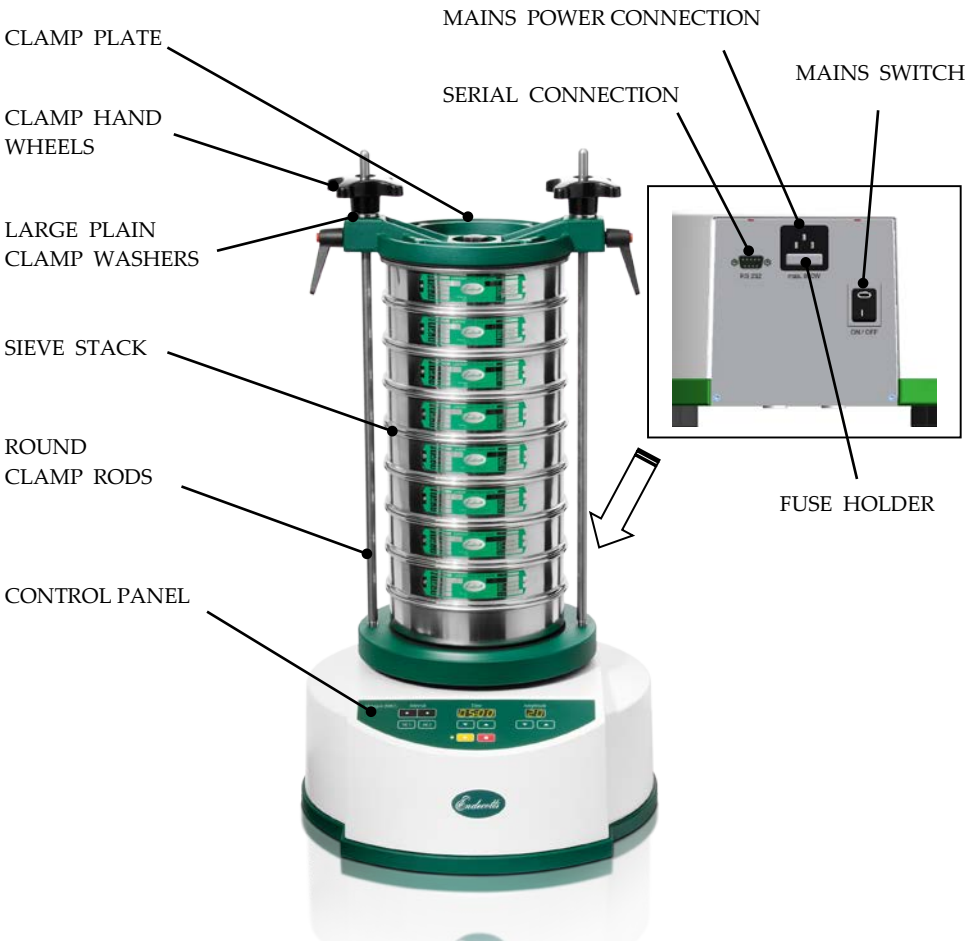

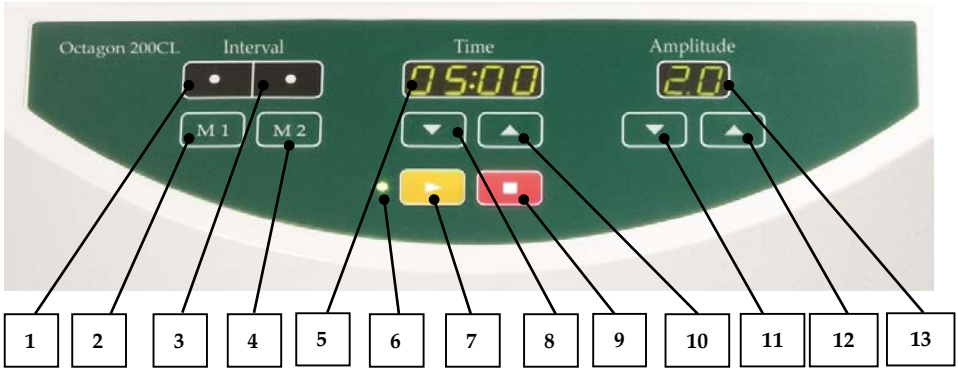

1 & 3	LED light to indicate chosen interval operation, ON.
2	Interval mode button M1 switches interval operation ON/OFF, upper LED lights up – 1 second on, 1 second off.
3	Interval mode button M2 switches interval operation ON/OFF, upper LED lights up – 10 seconds on, 2 seconds off.
5	Display shows the preselected sieving time, 00:10 – 99:50 sec's.
6	LED light to indicate START button ">" ON.
7	Start the machine by pressing the START button ">".
8 & 10	"v" and "^" button reduces/increases the sieving time, 00:10 – 99:50 min.
9	Stop the machine by pressing the STOP button "□".
11 & 12	"v" and "^" button reduces/increases the amplitude, 0.20 – 3.00mm, with digital display
13	Display amplitude shows the amplitude of 0.20 – 3.00mm

Setting Up

Electrical connections

- * The voltage and frequency for the **Octagon 200CL** is given on the rating label.
- * Ensure that the values agree with the existing power supply.
- * Connect the **Octagon 200CL** to the power supply using the connection cable provided.
- * When connecting the power cable to the mains external fusing is necessary according to the regulations of the installation location



Do not connect to any other supply other than stated on the rating label, otherwise electrical and mechanical components can be damaged.

Ambient temperature: 5°C to 40°C



If the ambient temperature is exceeded or drops below the specified value the electrical and mechanical components may become damaged and the performance data can change to an unknown degree.


Atmospheric humidity:

Maximum relative humidity 80% at temperatures up to 31°C, with linear reduction down to 50% relative humidity at 40°C.



At high atmospheric humidity the electrical and mechanical components may become damaged and the performance data can change to an unknown degree.

Transport protection

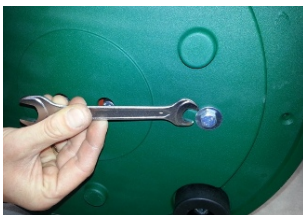

Place the **Octagon 200CL** on a stable laboratory bench, since otherwise unpleasant vibrations will be transmitted. Being placed on a level surface ensures symmetrical distribution of the sample over the sieves, during operation.

- Unscrew the two hexagon screws (transit bolts) on the bottom of the sieve shaker with an open ended spanner until the sieve plate is movable.
- Keep hexagon screws (transit bolts) for possible transport at a later date.




If the machine is operated with **the transit bolts**, or is transported without transit bolts, mechanical components may become damaged.

Reusing transit bolts

- Dismount the clamping unit.
- Screw the hexagon screws (transit bolts) into the two holes on the bottom of the sieve shaker and tighten with open ended spanner until the sieve plate is no longer movable.

Mount sieve clamping unit

Fit one M12 nut onto each clamp rod selected for use, then screw the pair of clamp rods into the location plate and tighten the locknuts.

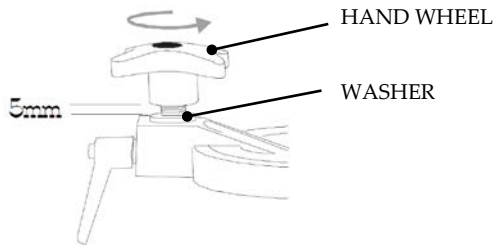

Place the two large plain washers over the 20mm threads of the clamp sleeves. These can be seen protruding vertically from the two side lugs on the clamp plate. Screw the two hand wheels loosely onto the 20mm threads; leave a gap of 5 mm between the large washer and the hand wheel face. Do not tighten right down at this point.

Operating Instructions



- 1 Place the receiver centrally on the location plate in the appropriate recess.
- 2 Stack the required test sieves on top of the receiver.
- 3 Put the sample in the top sieve and fit the lid

In order to guarantee exact results under fast sieving conditions, the quantity of material to be sieved should be adapted to the sieve diameter and the nominal mesh size.

More detailed information is displayed in our “TEST SIEVING MANUAL”.

- 4 Align the locking assemblies in figure 1 the two side lugs of the clamp plate with the round clamp rods. Slide the clamp plate down squarely onto the lid at the top of the sieve stack.

Ensure that the clamping hand wheels at the top (figure 2) are loose and the locking assemblies are fully pushed down. There should be a 5mm gap between the large plain washer and the face of the hand wheel.

Place one hand on the top of the clamp plate (figure 3) and hold square while locking one side handle lever. Repeat for the opposite side handle lever.


The side handle levers can be set vertically downwards by pressing on the Red button and pulling the handle outwards to release (figure 4). Turn the handle to a safe, convenient angle downwards and

1. Setting up

release to engage the teeth. Screw the two clamping hand wheels down simultaneously to ensure the clamping plate is square.

Continue until the hand wheels are tight against the internal stop. Hand tightness must be exerted so that the assembly does not loosen during vibration.

The locking side handle levers and clamping hand wheels must be tightened sufficiently to ensure that the sieves and receiver are clamped securely during operation.

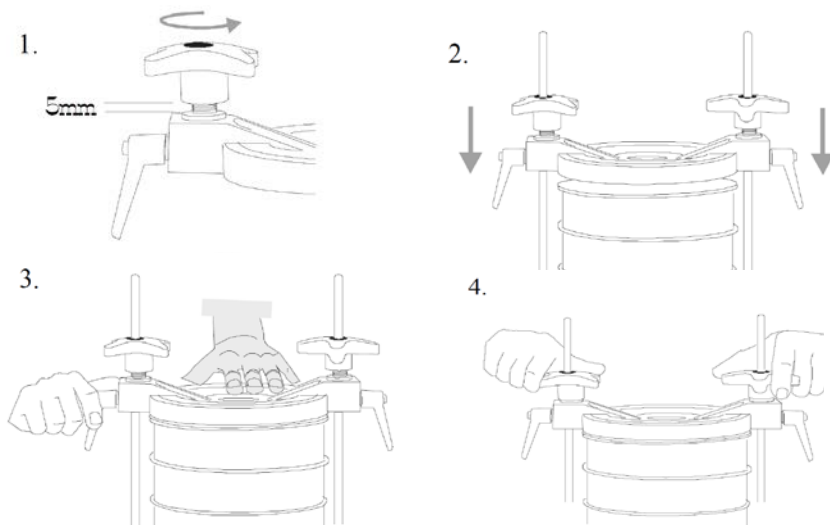

5 Set time, interval and amplitude

6 Press START



Damage may occur if the shaker is allowed to operate with a loose clamping plate.

Wet sieving

The Wet Sieving Adaptor Kit is supplied as an optional extra for 200 mm or 8” diameter sieves and should be ordered separately.

The Wet Sieving Adaptor Kit consists of the following items:

- 1 off Special Wet Sieving Clamp Plate.
- 1 Set off O-ring Seals (One required for each sieve in the stack.)
- 1 off Special Wet Sieving Receiver with a spout (Specify for 200 mm or 8” diameter sieves)



The O-ring seals are fitted on to the outside of the bottom rim of each sieve, which means the sieves are stacked onto each other and they form a seal.

The bottom sieve is placed on the special receiver with a spout.

A nylon hose tail must be fitted and must have a suitable length of hose fitted to drain into a convenient drainage point.

Fit a suitable length of hose to the spout to drain into a convenient drainage point.

The clamp plate is usually supplied with the rose reversed to avoid damage. Undo and reverse, so that the rose head is on the inside. Remove the lid from the sieve stack and replace the standard clamp plate with the wet sieving clamp plate. Fit a suitable length of hose to the inlet of the rose on the clamp plate and connect to the fluid supply with flow regulation.



Never operate your **Sieve shaker** directly in water.
Danger through current surge.



During wet sieving always operate your **Sieve shaker** connected to a mains socket protected by an FI protective (safety) switch.



The water quantity added should always be dosed in such a way that the sieve surface is only just wetted.



WHEN PARTICLE SIZE MATTERS

CERTIFICATE OF CE-CONFORMITY

TEST SIEVE SHAKER OCTAGON 200CL

Certificate of CE-Conformity according to:

EC Mechanical Engineering Directive 2006/42/EC

Applied harmonized standards, in particular:

EN ISO 12100 Security of machines

EC Directive Electromagnetic Compatibility 2004/108/EC

Applied standards, in particular:

EN55011:2009+A1:2010, Group 1, Class B Radio disturbance characteristics –
Limits and methods of measurement

EN 61000-3-2:2006+A1:2009+A2:2009

EN 61000-3-3:2008

EN61326-1:2006

Additional applied standards, in particular

EN 61010 Safety prescriptions concerning measuring, operating, controlling and laboratory equipment

Authorised for the compilation of technical documents:

Endecotts Ltd (technical documentation)

The following records are held by Endecotts Ltd in the form of Technical Documentation:

Detailed records of engineering development, construction plans, study (analysis) of the measures required for conformity assurance, analysis of the residual risks involved and operating instructions in due form according to the approved regulations for preparation of user information data.

The CE-conformity of the Endecotts Test Sieve Shaker Type Octagon 200CL is assured herewith.

In case of a modification to the machine not previously agreed with us as well as the use of not licensed spare parts and accessories this certificate will lose its validity.

Endecotts Ltd

London, July 2016

